


STRUCTURAL HEART SOLUTIONS

AMPLATZER™ SEPTAL OCCLUDERS



Information contained herein for **DISTRIBUTION outside of the U.S. ONLY.**
Always check the regulatory status of the device in your region.

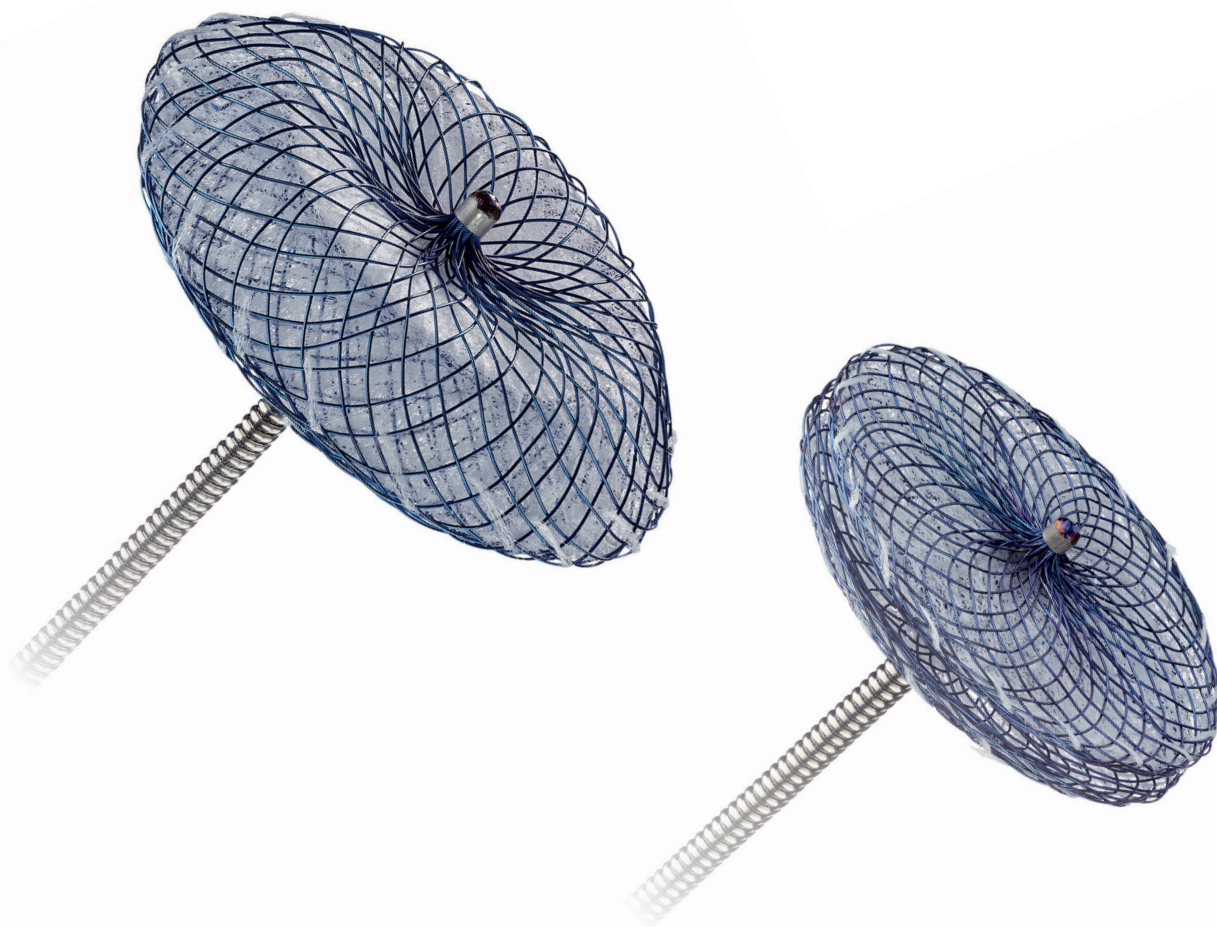

THE PROVEN STANDARD

FOR TRANSCATHETER ATRIAL SEPTAL DEFECT CLOSURE^{1, 2}

Amplatzer™ Septal Occluders are the standard of care for minimally invasive atrial septal defect (ASD) closure. These double-disc occluders are comprised of Nitinol mesh with polyester fabric. They are designed to securely appose the septal wall on each side of the defect and create a platform for tissue in-growth after implantation.

Information contained herein for **DISTRIBUTION outside of the U.S. ONLY**.
Always check the regulatory status of the device in your region.

WHEN SIMPLICITY MATTERS

The primary treatment option for closure of secundum atrial septal defects is with transcatheter devices.² This is when trust and simplicity matter. The Amplatzer™ Septal Occluder is the proven standard of care in transcatheter ASD closure.^{1,2}

SAFETY IN NUMBERS

98.5% Closure Rate: With no significant residual shunt (less than 2 mm) at 1-year follow-up¹

Low Major and Minor Complication Rates:

Postprocedure and long-term based on 5-year follow-up¹


SPECIFICALLY DESIGNED FOR ASD CLOSURE

Wide Waist: Centers device and fills the ASD³

Shape-memory Nitinol Mesh: Designed to securely appose both sides of the septal wall³

Polyester Material: Promotes occlusion and tissue in-growth³

Precise Placement: Device can be easily recaptured and redeployed³

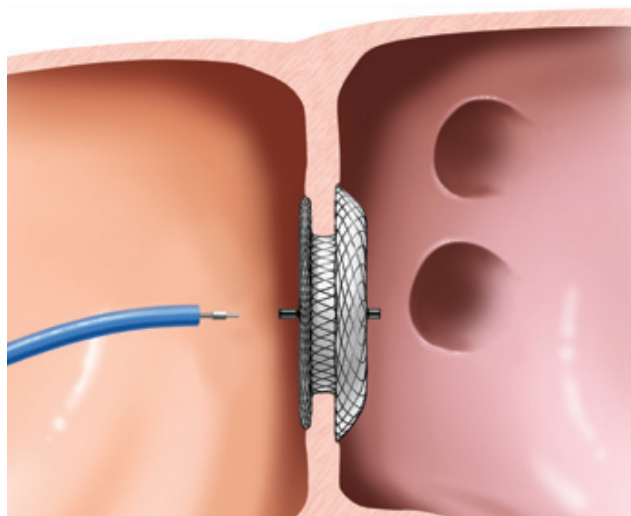

The waist of the Amplatzer™ Septal Occluder fills the defect for optimal occlusion.

WHEN FLEXIBILITY MATTERS

Not all septal defects are the same. They come in a variety of shapes, sizes and often there can be multiple communications between the left and right atria. These types of atrial septal defects require a special device designed with the flexibility to meet multiple needs.

The addition of the Amplatzer™ Multifenestrated Septal Occluder - “Cribriform” to the Amplatzer™ family of occluders enables transcatheter closure for the majority of atrial septal defects.


SPECIFICALLY DESIGNED FOR MULTIFENESTRATED ASD CLOSURE

Narrow Waist: Allows for placement through a central defect³

Matched Disc Diameters: Maximizes coverage of multiple fenestrations³

Polyester Material: Promotes occlusion and tissue in-growth³

Precise Placement: Device can be easily recaptured and redeployed³

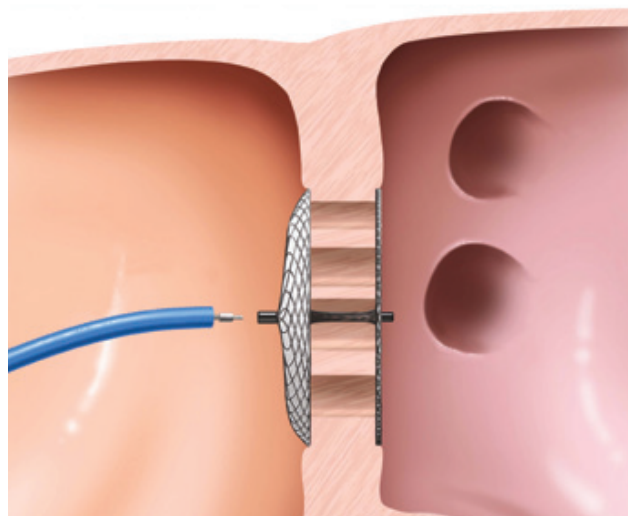

The Amplatzer™ Multifenestrated Septal Occluder - “Cribriform” enables occlusion of the defect by covering the fenestrations with a single device.

Stocking both the **Amplatzer™ Septal Occluder** and the **Amplatzer™ Multifenestrated Septal Occluder - “Cribriform”** provides you the ability to choose the appropriate device for a wide size-range of defects.

ORDERING INFORMATION

AMPLATZER™ SEPTAL OCCLUDER

| Model / Reorder Number | Waist Diameter (mm) | Waist Width (mm) | Right Atrial Disc Diameter (mm) | Left Atrial Disc Diameter (mm) |
|------------------------|---------------------|------------------|---------------------------------|--------------------------------|
| 9-ASD-004 | 4 | 3 | 12 | 16 |
| 9-ASD-005 | 5 | 3 | 13 | 17 |
| 9-ASD-006 | 6 | 3 | 14 | 18 |
| 9-ASD-007 | 7 | 3 | 15 | 19 |
| 9-ASD-008 | 8 | 3 | 16 | 20 |
| 9-ASD-009 | 9 | 3 | 17 | 21 |
| 9-ASD-010 | 10 | 3 | 18 | 22 |
| 9-ASD-011 | 11 | 4 | 21 | 25 |
| 9-ASD-012 | 12 | 4 | 22 | 26 |
| 9-ASD-013 | 13 | 4 | 23 | 27 |
| 9-ASD-014 | 14 | 4 | 24 | 28 |
| 9-ASD-015 | 15 | 4 | 25 | 29 |
| 9-ASD-016 | 16 | 4 | 26 | 30 |
| 9-ASD-017 | 17 | 4 | 27 | 31 |
| 9-ASD-018 | 18 | 4 | 28 | 32 |
| 9-ASD-019 | 19 | 4 | 29 | 33 |
| 9-ASD-020 | 20 | 4 | 30 | 34 |
| 9-ASD-022 | 22 | 4 | 32 | 36 |
| 9-ASD-024 | 24 | 4 | 34 | 38 |
| 9-ASD-026 | 26 | 4 | 36 | 40 |
| 9-ASD-028 | 28 | 4 | 38 | 42 |
| 9-ASD-030 | 30 | 4 | 40 | 44 |
| 9-ASD-032 | 32 | 4 | 42 | 46 |
| 9-ASD-034 | 34 | 4 | 44 | 50 |
| 9-ASD-036 | 36 | 4 | 46 | 52 |
| 9-ASD-038 | 38 | 4 | 48 | 54 |
| 9-ASD-040 | 40 | 4 | 50 | 56 |

AMPLATZER™ MULTIFENESTRATED SEPTAL OCCLUDER - “CRIBRIFORM”

| Model / Reorder Number | Right & Left Atrium Disc Diameter (mm) | Waist Width (mm) |
|------------------------|--|------------------|
| 9-ASD-MF-018 | 18 | 3 |
| 9-ASD-MF-025 | 25 | 3 |
| 9-ASD-MF-030 | 30 | 3 |
| 9-ASD-MF-035 | 35 | 3 |
| 9-ASD-MF-040 | 40 | 3 |

REFERENCE:

- Amplatzer Septal Occluder Instructions for Use.
- Kashour TS, Latroche B, Elhoury ME, et al. Successful Percutaneous Closure of a Secundum Atrial Septal Defect through Femoral Approach in a Patient with Interrupted Inferior Vena Cava. *Congenital Heart Disease*. 2010;5(6):620-623.
- Test(s) performed by and data on file at Abbott.

CAUTION: This product is intended for use by or under the direction of a physician. Prior to use, reference the Instructions for Use, inside the product carton (when available) or at eifu.abbottvascular.com or at medical.abbott/manuals for more detailed information on Indications, Contraindications, Warnings, Precautions and Adverse Events.

Information contained herein for **DISTRIBUTION outside of the U.S. ONLY**. Always check the regulatory status of the device in your region.

Illustrations are artist's representations only and should not be considered as engineering drawings or photographs. Photo(s) on file at Abbott.

Abbott

3200 Lakeside Dr. Santa Clara, CA 95054

™ Indicates a trademark of the Abbott group of companies.

‡ Indicates a third-party trademark, which is property of its respective owner.

www.structuralheart.abbott

©2023 Abbott. All rights reserved. MAT-2004327 v2.0 | Item approved for OUS use only.

